



F405@+1000V, T9 setup5 CH3, signal

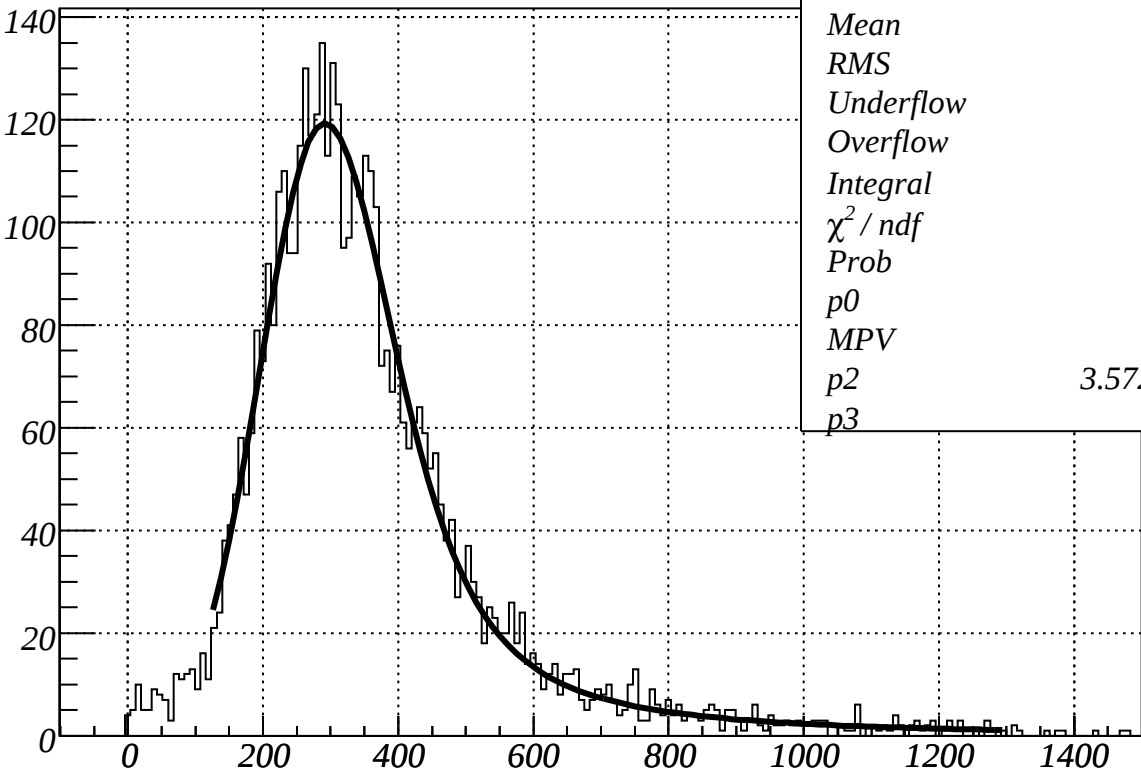

F405 T11 setup5, signal	
Entries	4479
Mean	357.5
RMS	186.4
Underflow	0
Overflow	0
Integral	4464
χ^2 / ndf	114.5 / 134
Prob	0.8874
p0	28.25 ± 1.55
MPV	261.7 ± 2.4
p2	$3.572e+04 \pm 560$
p3	79.7 ± 3.7

F405@+1000V, T9 setup5 CH3, noise

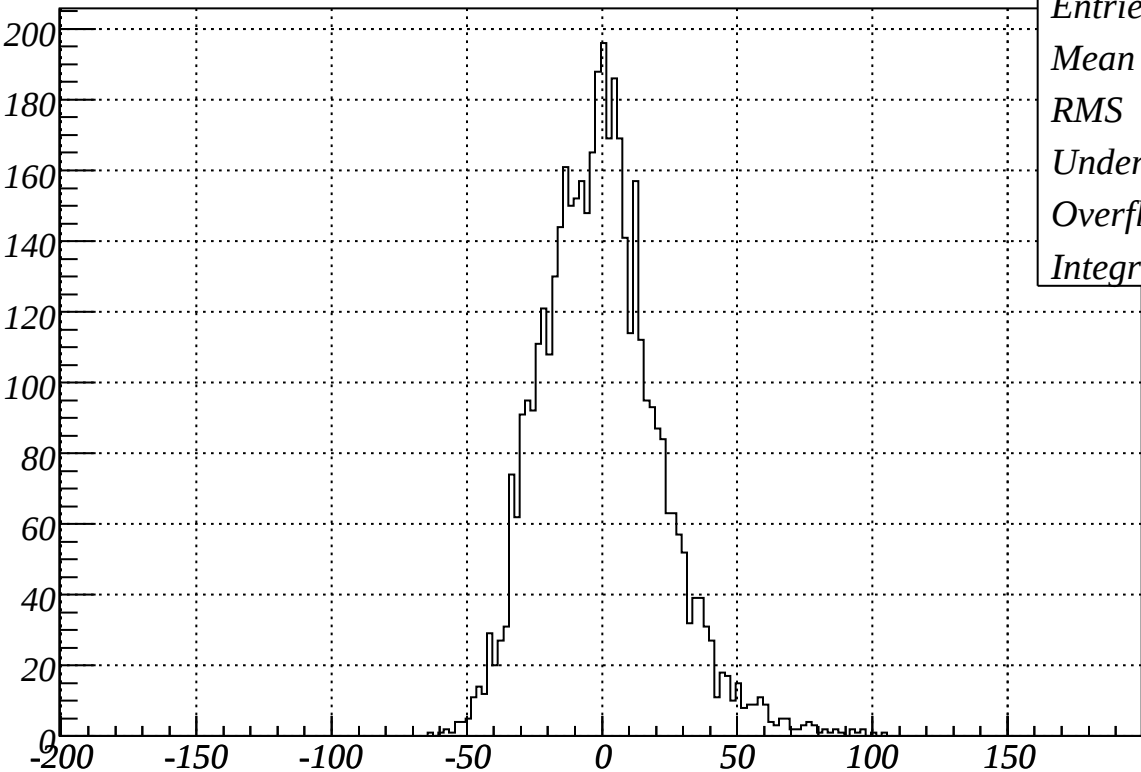

F405 T11 setup5, noise	
Entries	4479
Mean	-0.3515
RMS	21.87
Underflow	0
Overflow	0
Integral	4479