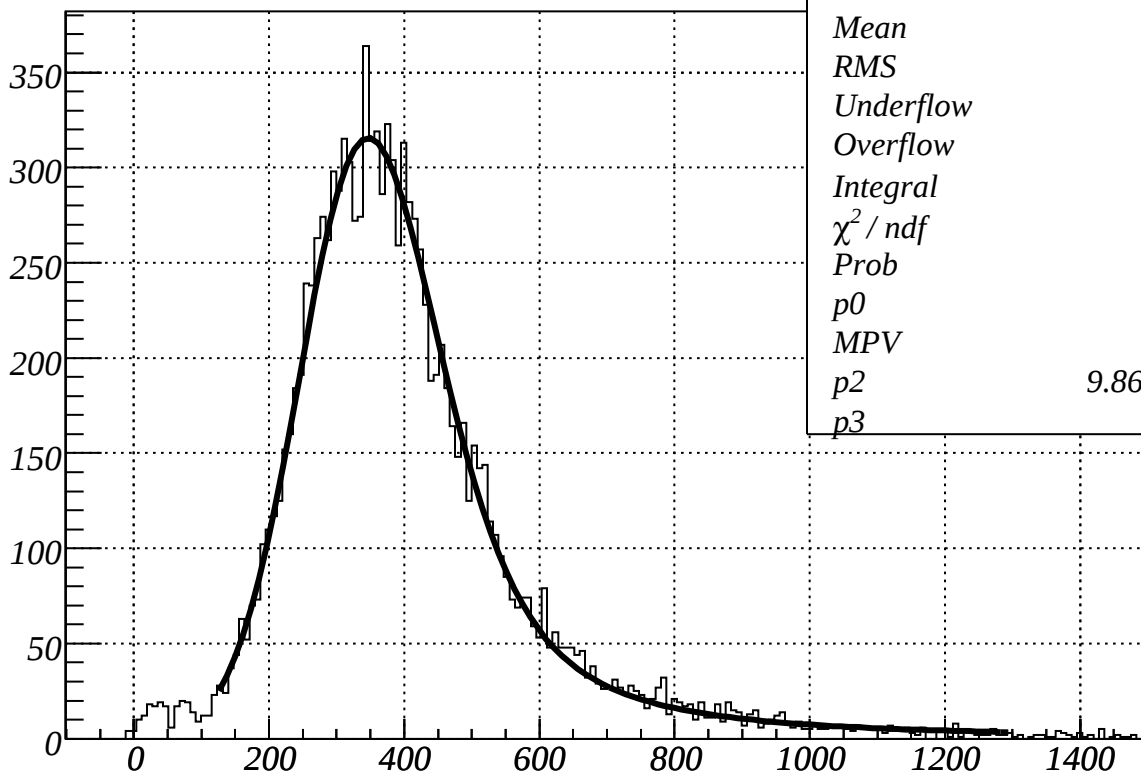
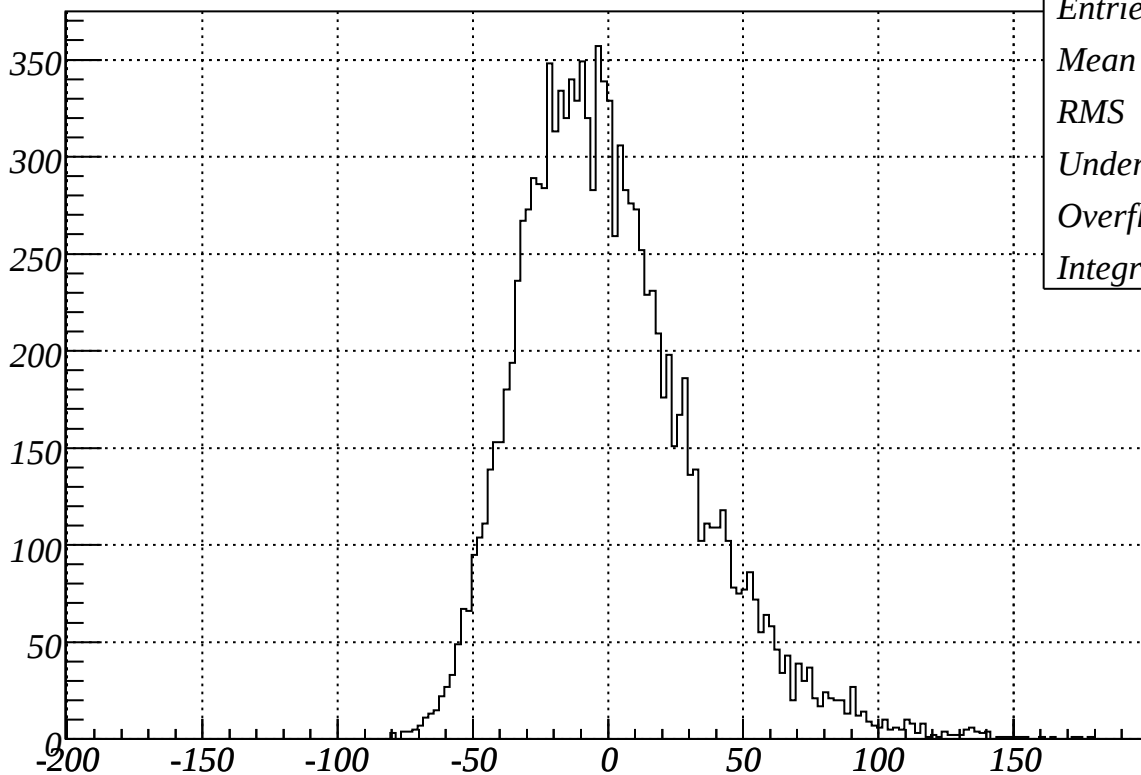


F405@+1000V, T9 setup1 CH3, signal*F405 T9 setup1, signal*

Entries	12301
Mean	405.2
RMS	184.5
Underflow	0
Overflow	0
Integral	1.228e+04
χ^2 / ndf	178 / 141
Prob	0.01898
p0	27.76 ± 0.91
MPV	315.1 ± 1.5
p2	9.861e+04 ± 913
p3	85.97 ± 1.79

F405@+1000V, T9 setup1 CH3, noise*F405 T9 setup1, noise*

Entries	12301
Mean	0.2676
RMS	32.56
Underflow	0
Overflow	0
Integral	1.23e+04