



F407@-1000V, T9 setup3 CH1, signal

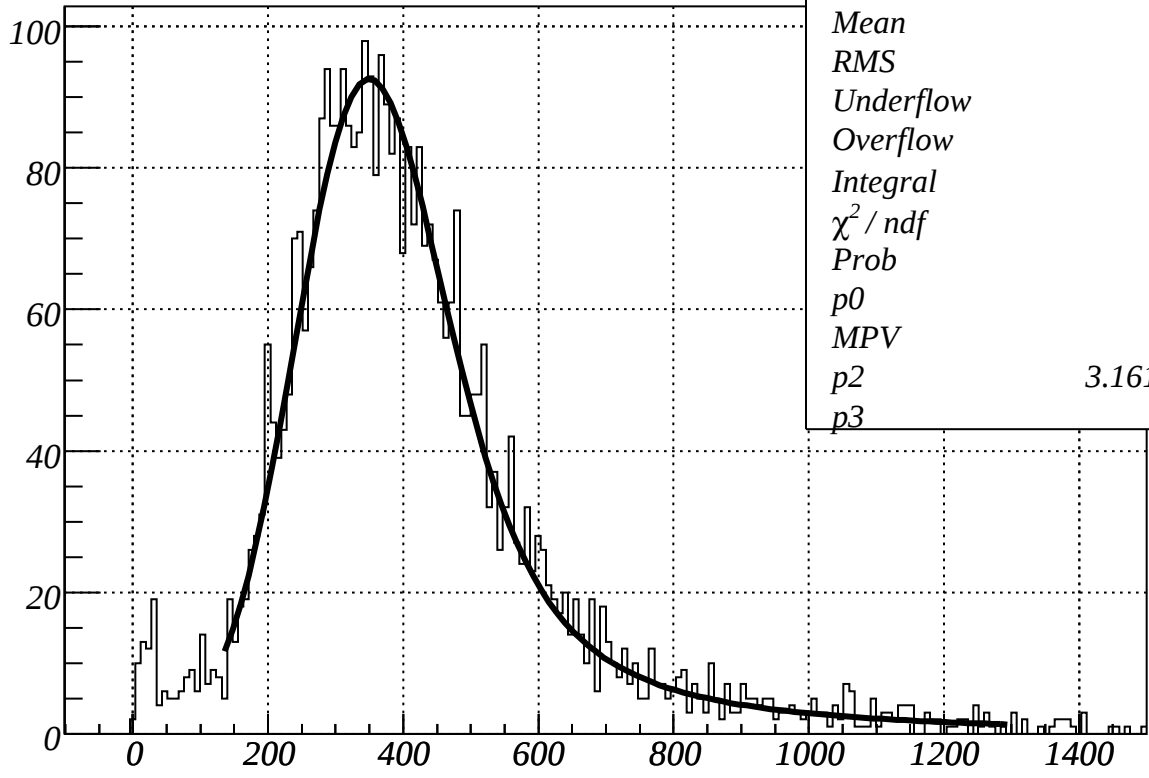

F407 T9, signal	
Entries	4056
Mean	416.2
RMS	208.5
Underflow	0
Overflow	0
Integral	4034
χ^2 / ndf	130.2 / 136
Prob	0.6241
p0	32.99 ± 1.97
MPV	315.3 ± 3.1
p2	$3.161\text{e}+04 \pm 529$
p3	89.57 ± 3.97

F407@-1000V, T9 setup3 CH1, noise

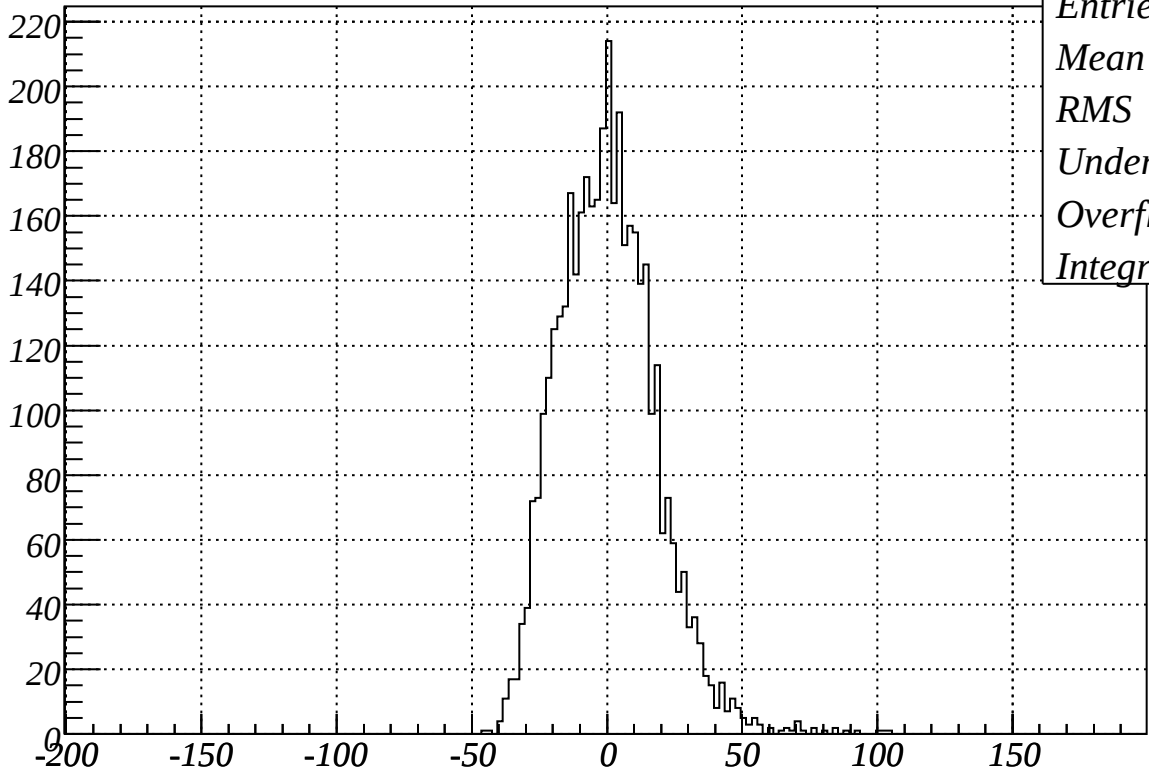

F407 T9, noise	
Entries	4056
Mean	0.2821
RMS	17.84
Underflow	0
Overflow	0
Integral	4056