



## Performance study of silicon photomultipliers as photon detectors for PET

R. Verheyden<sup>a,\*</sup>, H. Chagani<sup>a</sup>, R. Dolenec<sup>a</sup>, R. Pestotnik<sup>a</sup>, P. Križan<sup>a,b</sup>, S. Korpar<sup>a,c</sup>, A. Stanovnik<sup>a,d</sup><sup>a</sup> Jožef Stefan Institute, Jamova Cesta 39, Ljubljana 1000, Slovenia<sup>b</sup> Faculty of Mathematics and Physics, University of Ljubljana, Slovenia<sup>c</sup> Faculty of Chemistry and Chemical Engineering, University of Maribor, Slovenia<sup>d</sup> Faculty of Electrical Engineering, University of Ljubljana, Slovenia

## ARTICLE INFO

Available online 6 July 2010

## Keywords:

Positron emission tomography

Geiger mode APD

Silicon Photomultiplier

LYSO scintillator

## ABSTRACT

The use of Silicon Photo-Multipliers (SiPMs) as photon detectors in Positron Emission Tomography (PET) modules offers significant advantages over conventional light sensors, including application in a magnetic field, better resolution and easier operation. Different types of SiPMs have been tested: Photonique,  $2.1 \times 2.1 \text{ mm}^2$ , Hamamatsu  $3 \times 3 \text{ mm}^2$  and STMicroelectronics  $3.5 \times 3.5 \text{ mm}^2$ . Dark noise, surface sensitivity, photon detection efficiency and linearity at low light intensities have been measured. A LYSO crystal was coupled to a SiPM to test the performance as a photon detector for PET. We will present the results of the measurements for different samples and types.

© 2010 Elsevier B.V. All rights reserved.

## 1. Introduction

Positron Emission Tomography (PET) is a non-invasive method for in-depth and in vivo imaging of tissue. The positron emitted in a  $\beta^+$ -decay of the nucleus slows down in the tissue and subsequently annihilates with a nearby electron. The annihilation gamma-rays of 511 keV are usually detected indirectly, through scintillation in inorganic crystals. Photon detectors, like Photomultiplier Tubes (PMTs), detect the scintillation light. The majority of PET devices use PMTs, but due to their size, relatively poor ratio of active to total surface and high price, which is a significant fraction of the total cost of the device, it is worthwhile to search for alternative detectors of visible and infrared photons. The sensitivity of PMTs to magnetic fields and the increasing requirement to unify different image modalities in one measurement, provides an additional reason to search for new detectors. One would like to incorporate a PET apparatus inside a MRI magnet for simultaneous imaging of tissue function and density. A new type of semiconductor detector, the Silicon Photomultiplier (SiPM) looks very promising [1–4]. Results for the surface sensitivity, energy resolution and linearity, as well as timing resolution for several SiPM samples are presented.

## 2. Surface sensitivity

Surface sensitivity is assessed by exposing each SiPM to a pulsed  $\sim 5 \mu\text{m}$  wide laser beam. The SiPM is moved relative to the

light source to produce two-dimensional scans (Fig. 1) of the count rate over the surface of the silicon photomultiplier. Only SiPM pulses corresponding to the single photon pulse height and coincident with the laser pulse within a  $\sim 10 \text{ ns}$  time window are selected. Surface sensitivity for different SiPMs (Hamamatsu H100C, CPTA/Photonique S137 and STMicroelectronics) were measured and found that they are fairly uniform across their surfaces. More detailed surface scans of the SiPMs, shown in Fig. 1, reveal the pixelated structure of the SiPMs and reflect the internal structure of quenching resistors and diode cells for every SiPM.


The Hamamatsu H100C and CPTA/Photonique S137 SiPM used for the surface scans were  $1 \text{ mm} \times 1 \text{ mm}$  sized samples. However, larger sized samples of these companies use the same technology as the small ones so the results should be similar. It is important also to note that the SiPMs from STMicroelectronics have additional thin trenches filled with oxide and metal surrounding the individual cells. Such a trench serves to reduce the electro-optical coupling between individual micro-cells. One disadvantage of this trench is the reduction of the fill factor ( $\sim 36\%$ ) of this SiPM compared to SiPMs from other manufacturers (H100C  $\sim 75\%$  and S137  $\sim 60\%$ ).

## 3. Energy resolution


The energy resolution of the SiPMs has been measured by coupling a LYSO crystal from Sinocera [5] (Fig. 2) to the SiPMs and measuring the coincidence annihilation  $\gamma$ 's from a  $^{22}\text{Na}$  source. The LYSO crystal has a fast decay time (40–44 ns), a high light yield (75% of NaI), an intrinsic energy resolution of 20%, and a peak emission wavelength at 428 nm. The crystal was wrapped

\* Corresponding author.

E-mail address: [ruben.verheyden@ijs.si](mailto:ruben.verheyden@ijs.si) (R. Verheyden).

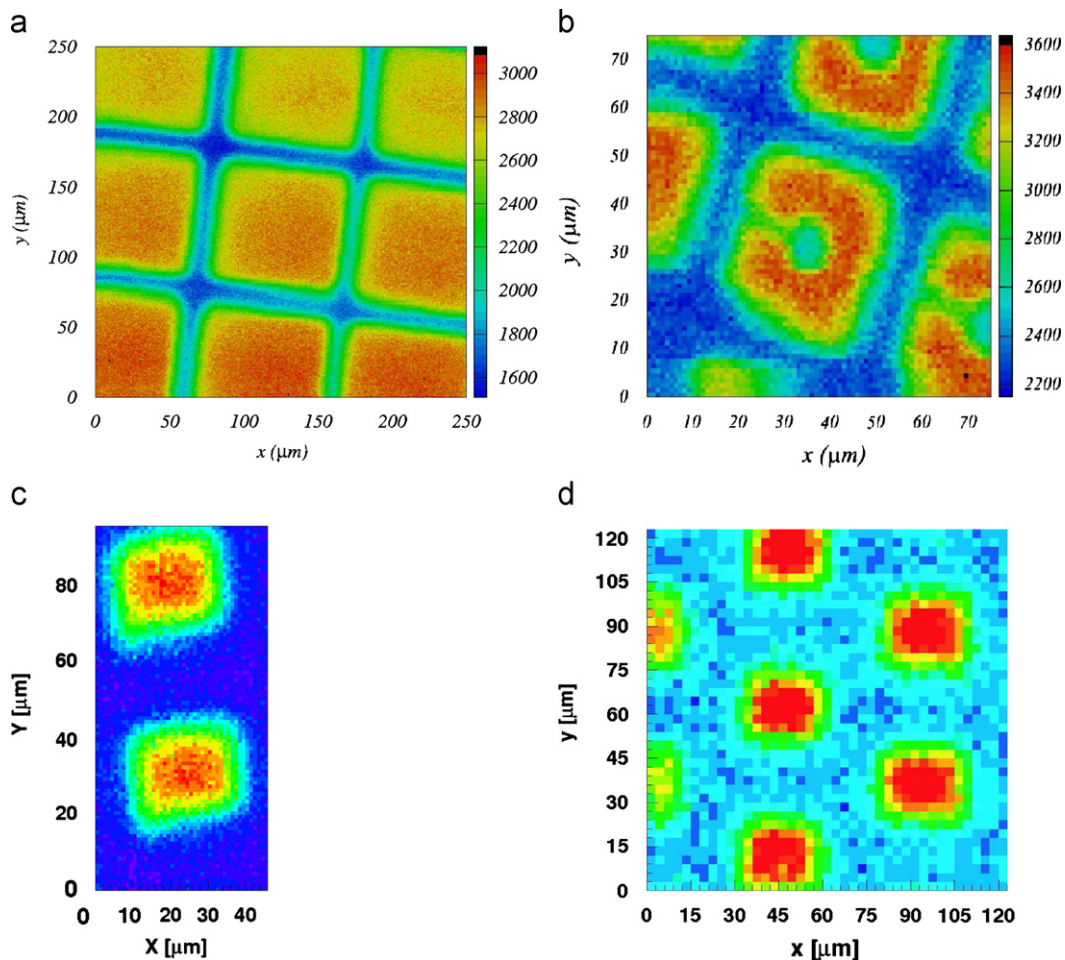

**Fig. 1.** Two-dimensional scans for (a) Hamamatsu H100C, (b) CPTA/Photonique and (c) and (d) STMicroelectronics. Surface scans are valuable to assess the surface sensitivity of SiPMs, (a)–(c) were performed with a step size of 1  $\mu\text{m}$  and clearly show the structure of individual SiPM cells. (d) shows a part of a larger surface scan (STMicroelectronics with a step size of 3  $\mu\text{m}$ ).



**Fig. 2.** Schematic of the setup used to measure the energy resolution of single SiPMs. A LYSO crystal coupled to a SiPM was used as triggering detector for the coincidence measurement.

with teflon and attached to the SiPM using optical grease to ensure a good optical coupling between the crystal and the SiPM. Fig. 3 shows the results for the three SiPMs, exhibiting a  $\sim 19\%$  FWHM for CPTA/Photonique and STMicroelectronics, and 10% FWHM for Hamamatsu H100C. The energy resolution measurements are limited due to the intrinsic energy resolution of the crystal. Note that the results for the energy resolution were not corrected for the non-linear behaviour due to the finite number of cells.

Photonique and STM offer smaller pitch ( $\sim 50 \times 50 \mu\text{m}^2$ ) compared to the used Hamamatsu H100C SiPM which has a larger cell size ( $100 \times 100 \mu\text{m}^2$ ). Hamamatsu also offers SiPMs with a smaller cell size, however a larger cell size, using the same technology, results in a higher geometrical efficiency (higher PDE) and higher gain (better timing). On the other hand, it also reduces the number of cells per  $\text{mm}^2$ , and thus effectively reduces also the dynamical range. This becomes manifest in the non-linear response of the Hamamatsu SiPM due to the total number of scintillation photons from the LYSO crystal exceeding the number

of cells as shown in Fig. 4a. For the Hamamatsu H100C ( $900 \text{ cells}/3 \times 3 \text{ mm}^2$ ) energy linearity was evaluated (see Fig. 4a) by measuring the energy spectrum for three different radioactive sources ( $^{22}\text{Na}$ ,  $^{137}\text{Cs}$ , and the  $^{176}\text{Lu}$  background of the LYSO crystal).


For the STMicroelectronics ( $4900 \text{ cells}/3.5 \times 3.5 \text{ mm}^2$ ) a uniform illumination from a laser was used to study the linearity. The laser light intensity was controlled by using neutral density filters.

The results for linearity of the Hamamatsu and STMicroelectronics samples (Figs. 4a and b) are in agreement with the expected behaviour due to the number of pixels. Devices with a larger number of pixels/ $\text{mm}^2$  provide a better linear response over a wider dynamic range.


#### 4. Timing resolution

In PET scanners, the time difference between two back-to-back photons yields information about the position of positron-electron annihilation in the patient's tissue. This information can be used to improve the imaging resolution due to much higher background rejection. Therefore, the accurate determination of the position of an event is dependent on the time resolution.

One of the issues is whether the intrinsic timing resolution of SiPMs limits the coincidence timing. Therefore the intrinsic timing resolution of two Silicon photomultipliers from different

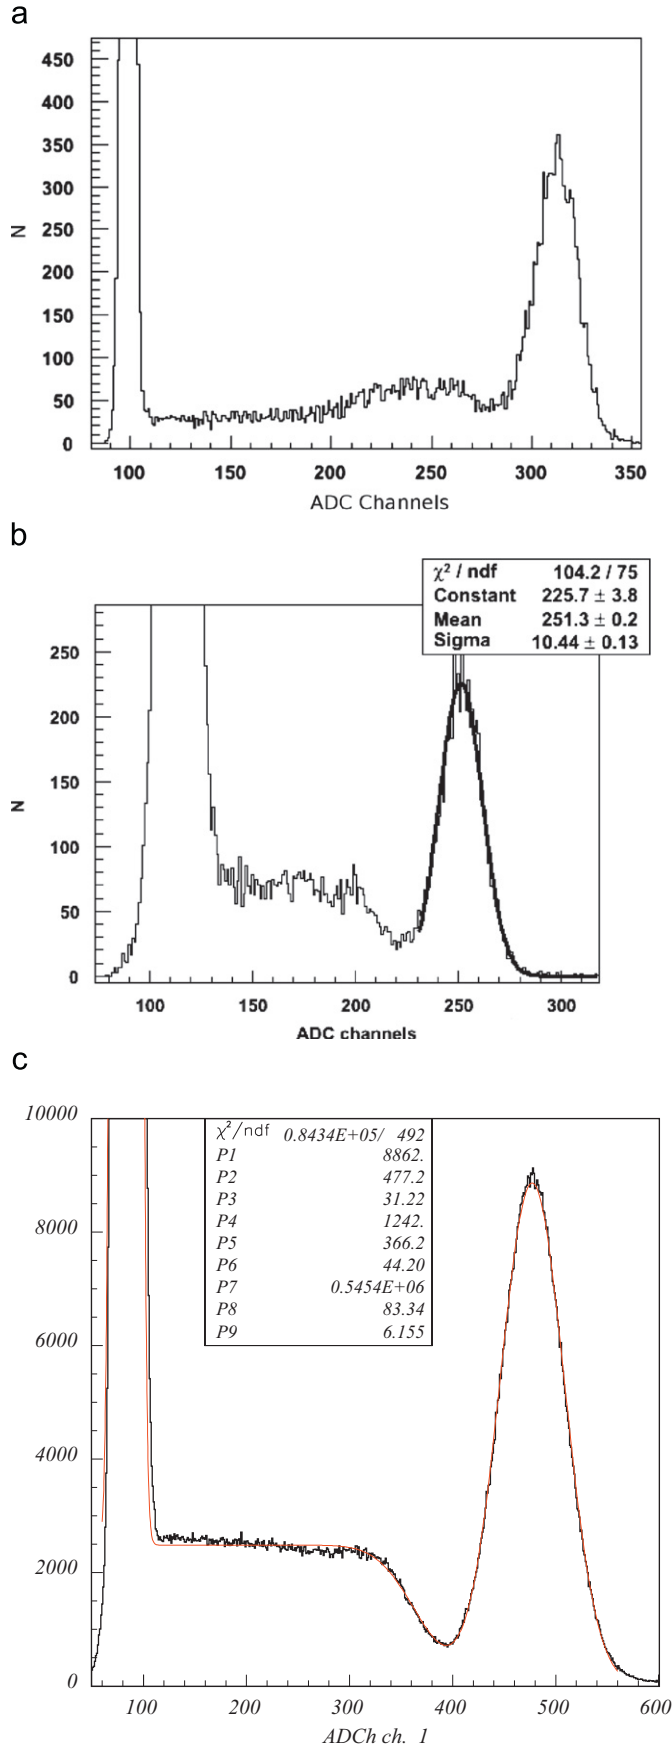

**Fig. 3.** Energy spectra for three different SiPMs: (a) Hamamatsu H100C. (b) CPTA/Photonique S137 and (c) STMicroelectronics.

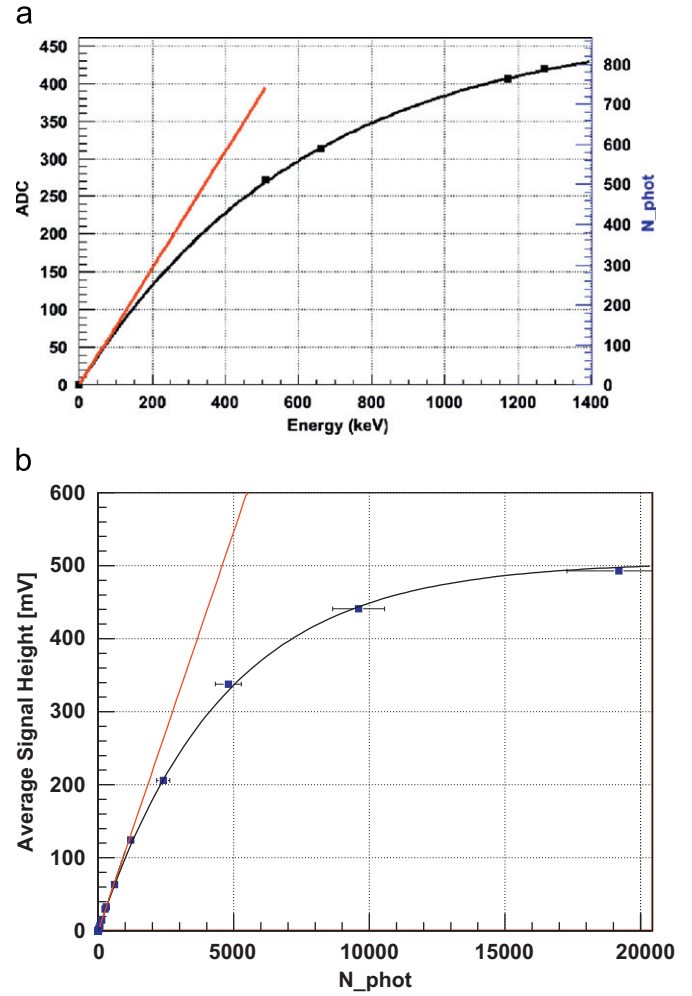

**Fig. 4.** Energy linearity for two different SiPMs: (a) Hamamatsu H100C clearly shows a non-linear behaviour. (b) The STMicroelectronics SiPM shows a good linearity up to several thousands of photons.

**Table 1**

The time resolution after time-walk correction for different SiPMs.

1 mm <sup>2</sup> SiPM	S137	H100C
$\sigma_{\text{red}}$ (ps)	182	145
$\sigma_{\text{blue}}$ (ps)	151	136

producers was measured by exposing the samples to very weak light pulses ( $\sim 10$  ps width) from a PILAS [6] laser. The laser light intensity was controlled with neutral density filters and was set to the single photon level.

Although not that fast as for example a microchannel plate PMT, the time resolution of the measured samples amounts to 100–200 ps (Table 1). The measurements of the time resolution at different wavelengths (blue 405 nm, and red 635 nm) show that the measured samples give a better time resolution in the blue light region. This makes them good candidates to be used together with the LYSO crystal (peak emission at 428 nm).

First measurements with Hamamatsu  $3 \times 3$  mm<sup>2</sup> SiPMs of back-to-back  $\gamma$ 's resulted in a timing resolution of  $\sim 442$  ps (Fig. 5). This result can be attributed to the expected slower behaviour of the used larger sample size due to its higher capacitance. This larger capacitance results in a slower rise-time which in turn worsens the timing resolution of the SiPM. Another

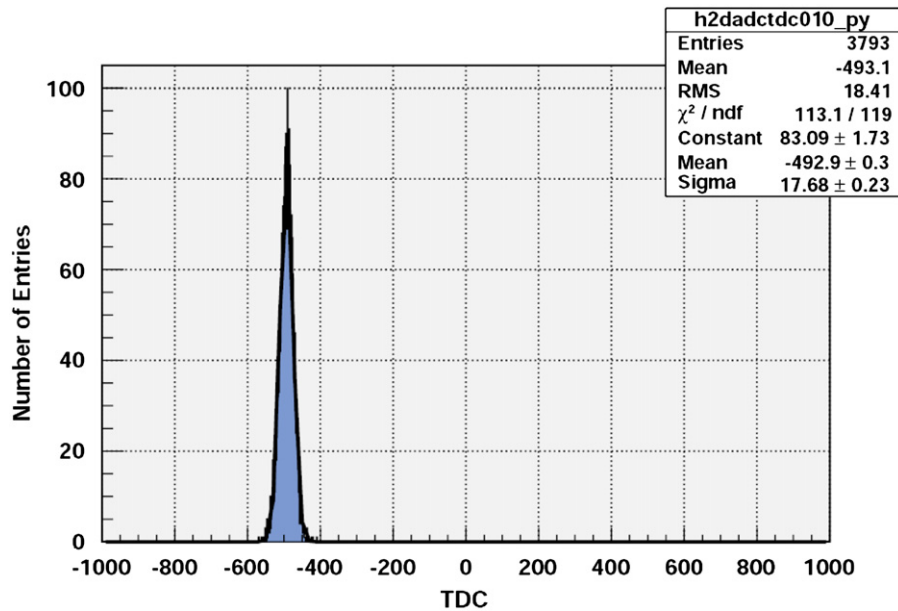


Fig. 5. Timing resolution for back-to-back  $\gamma$ 's (25 ps/bin  $\rightarrow \sigma_t \sim 442$  ps). Hamamatsu  $3 \times 3$  mm<sup>2</sup> SiPMs were used for this measurement.

limiting factor is a relatively high discrimination level at about 10 photo-electrons. Using fast pre-amplifiers with a wide dynamic range would enable the single photo-electron timing discrimination and improve the timing resolution.

## 5. Conclusions

Silicon photomultipliers seem to be a very promising detector for PET. The main advantages are their insensitivity for magnetic fields and their compactness. Surface sensitivity, energy resolution and timing resolution of several SiPMs have been evaluated. The relatively good energy resolution and fast response might enable to reduce the background in PET imaging and thus to

improve the resolution. Further studies will be performed using SiPMs in a PET module to assess the possibility of using SiPMs as photon detectors in a NMR-PET combination. All three measured SiPM samples show a reasonable performance to be used for PET.

## References

- [1] P. Buzhan, et al., An advanced study of Silicon Photomultiplier, ICFA Instrumentation Bulletin, Fall issue 2001.
- [2] B. Dolgoshein, et al., Nucl. Instr. and Meth. A 563 (2006) 368.
- [3] D. Renker, Nucl. Instr. and Meth. A 567 (2006) 48.
- [4] D. Renker, E. Lorenz, JINST 4 (2009) P04004.
- [5] [http://www.sinocera.net/en/crystal\\_lyso.asp](http://www.sinocera.net/en/crystal_lyso.asp).
- [6] <http://www.alsgmbh.com/>.